


# Effects of Sterilization and 1- & 3-Year Accelerated Aging on Material Tensile Strength (MD) for 1059B




Tyvek.

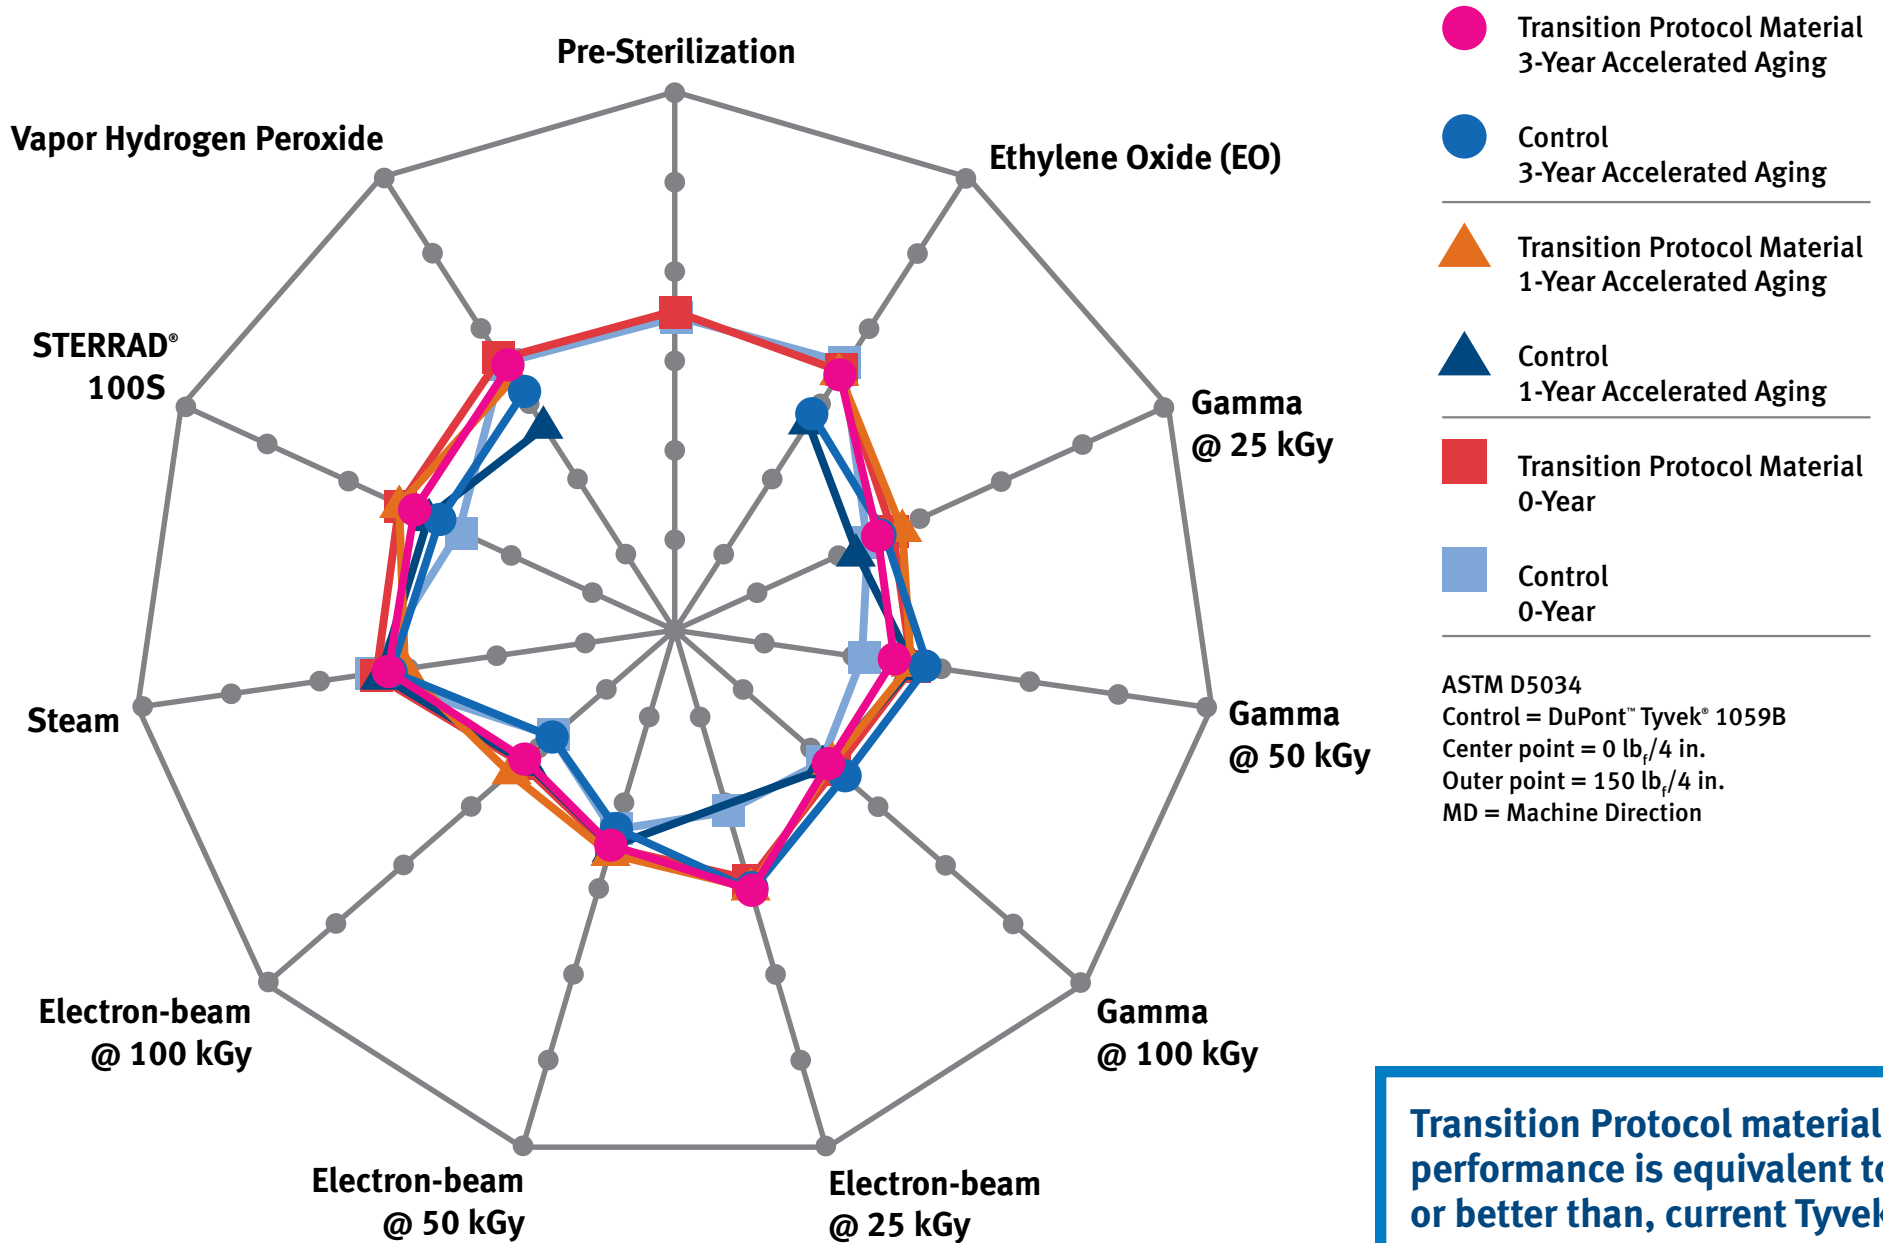

# Effects of Sterilization and 1- & 3-Year Accelerated Aging on Material Tensile Strength (CD) for 1059B




Tyvek.

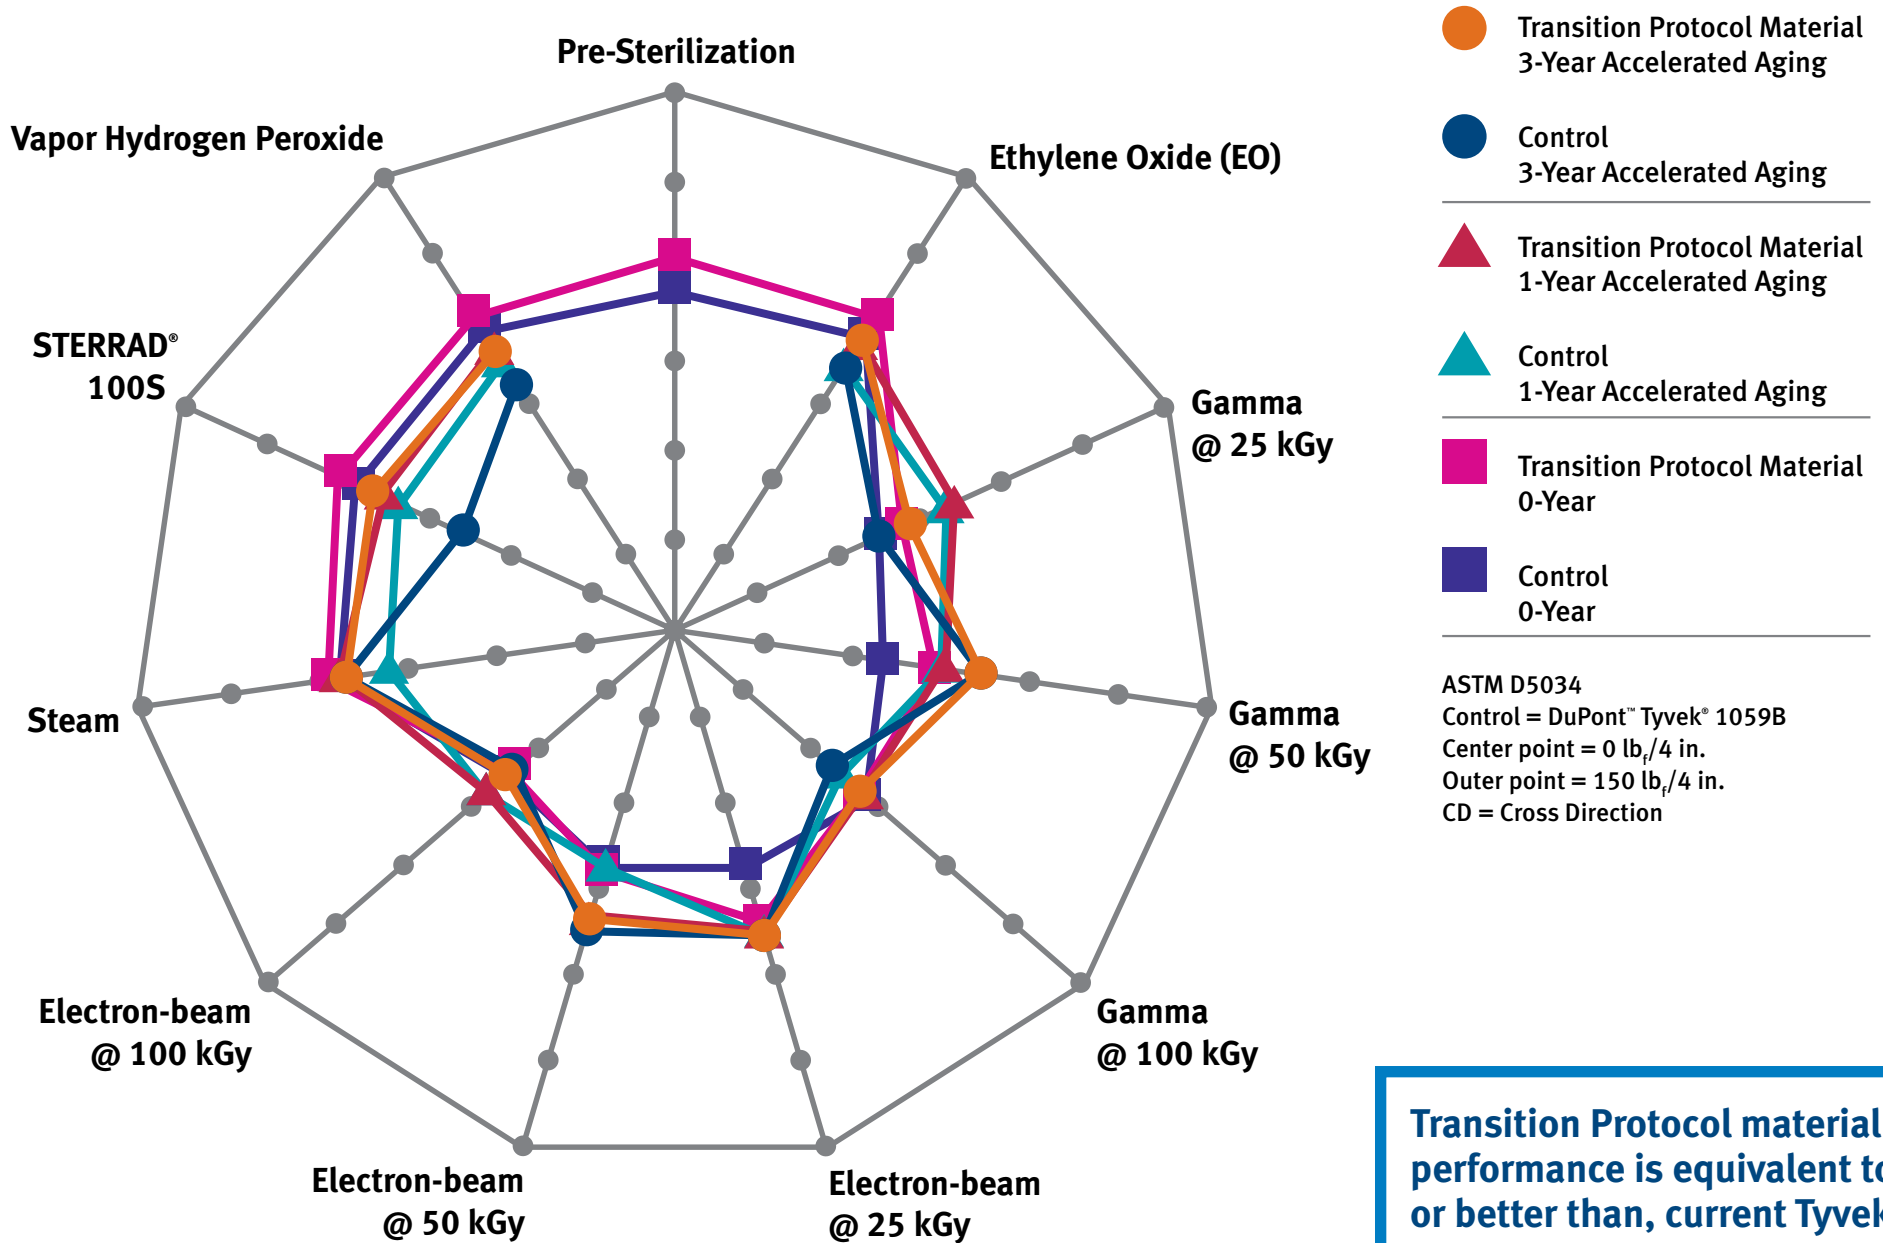

# Effects of Sterilization and 1- & 3-Year Accelerated Aging on Material Elongation (MD) for 1059B



Tyvek.

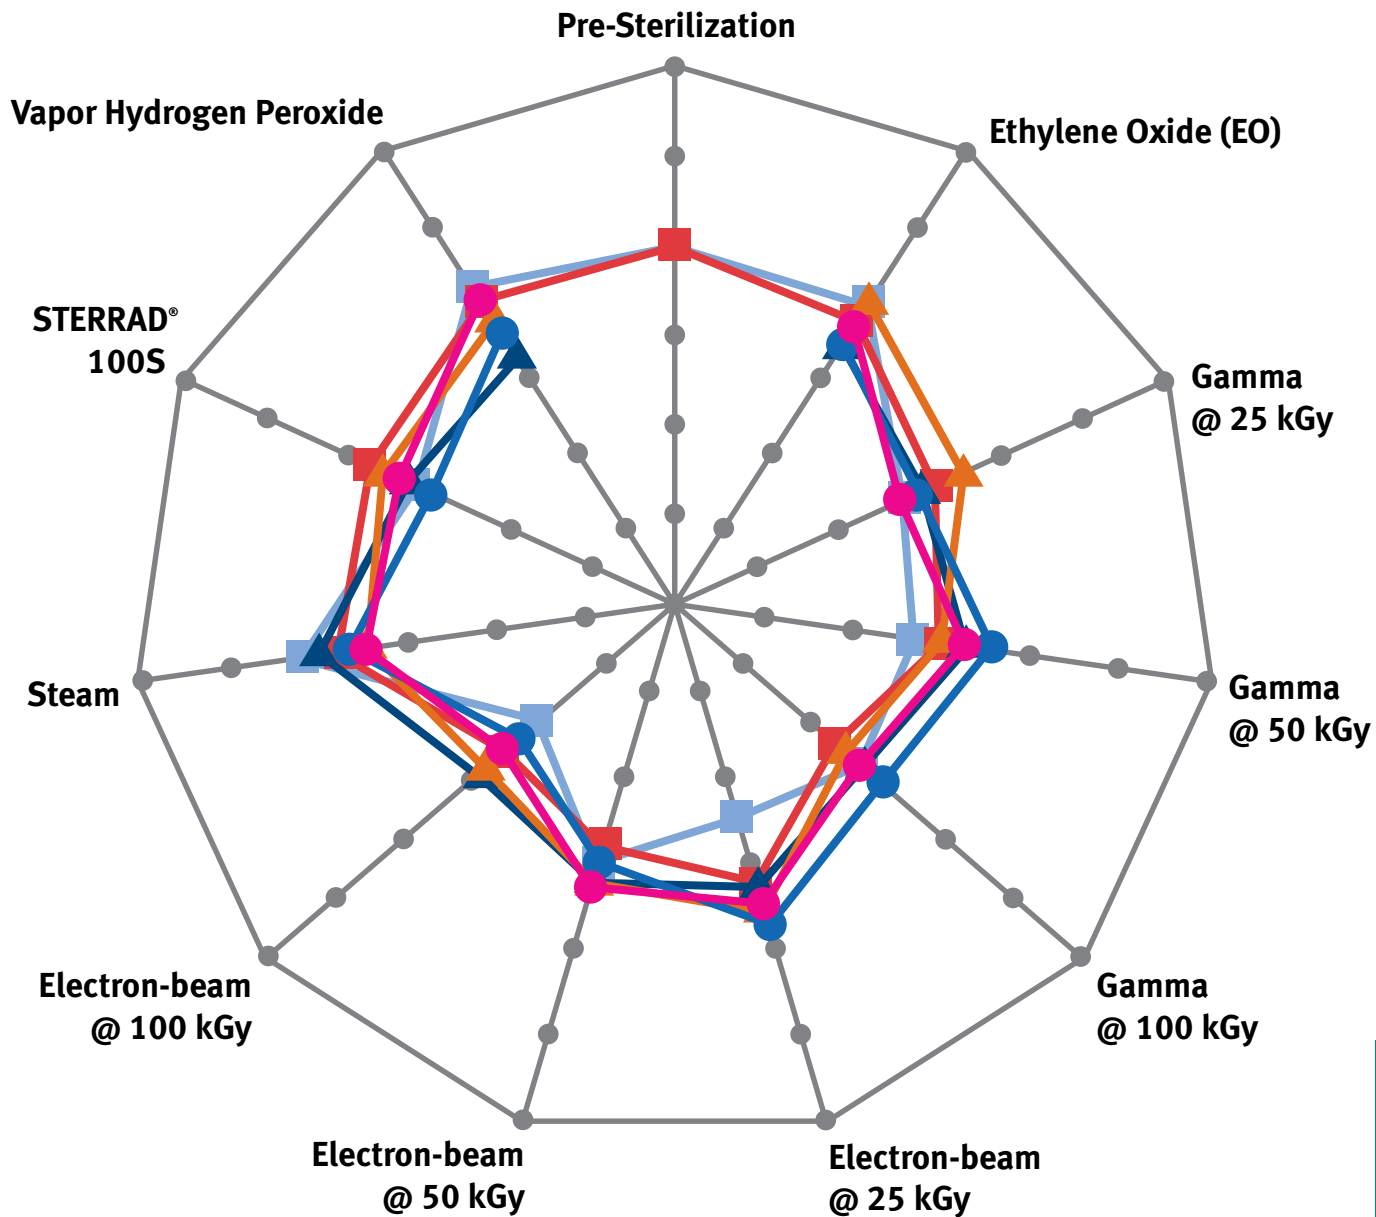

- Transition Protocol Material 3-Year Accelerated Aging
- Control 3-Year Accelerated Aging
- ▲ Transition Protocol Material 1-Year Accelerated Aging
- ▲ Control 1-Year Accelerated Aging
- Transition Protocol Material 0-Year
- Control 0-Year


ASTM D5034  
 Control = DuPont™ Tyvek® 1059B  
 Center point = 0%  
 Outer point = 30%  
 MD = Machine Direction

**Transition Protocol material performance is equivalent to, or better than, current Tyvek®.**

# Effects of Sterilization and 1- & 3-Year Accelerated Aging on Material Elongation (CD) for 1059B



Tyvek.

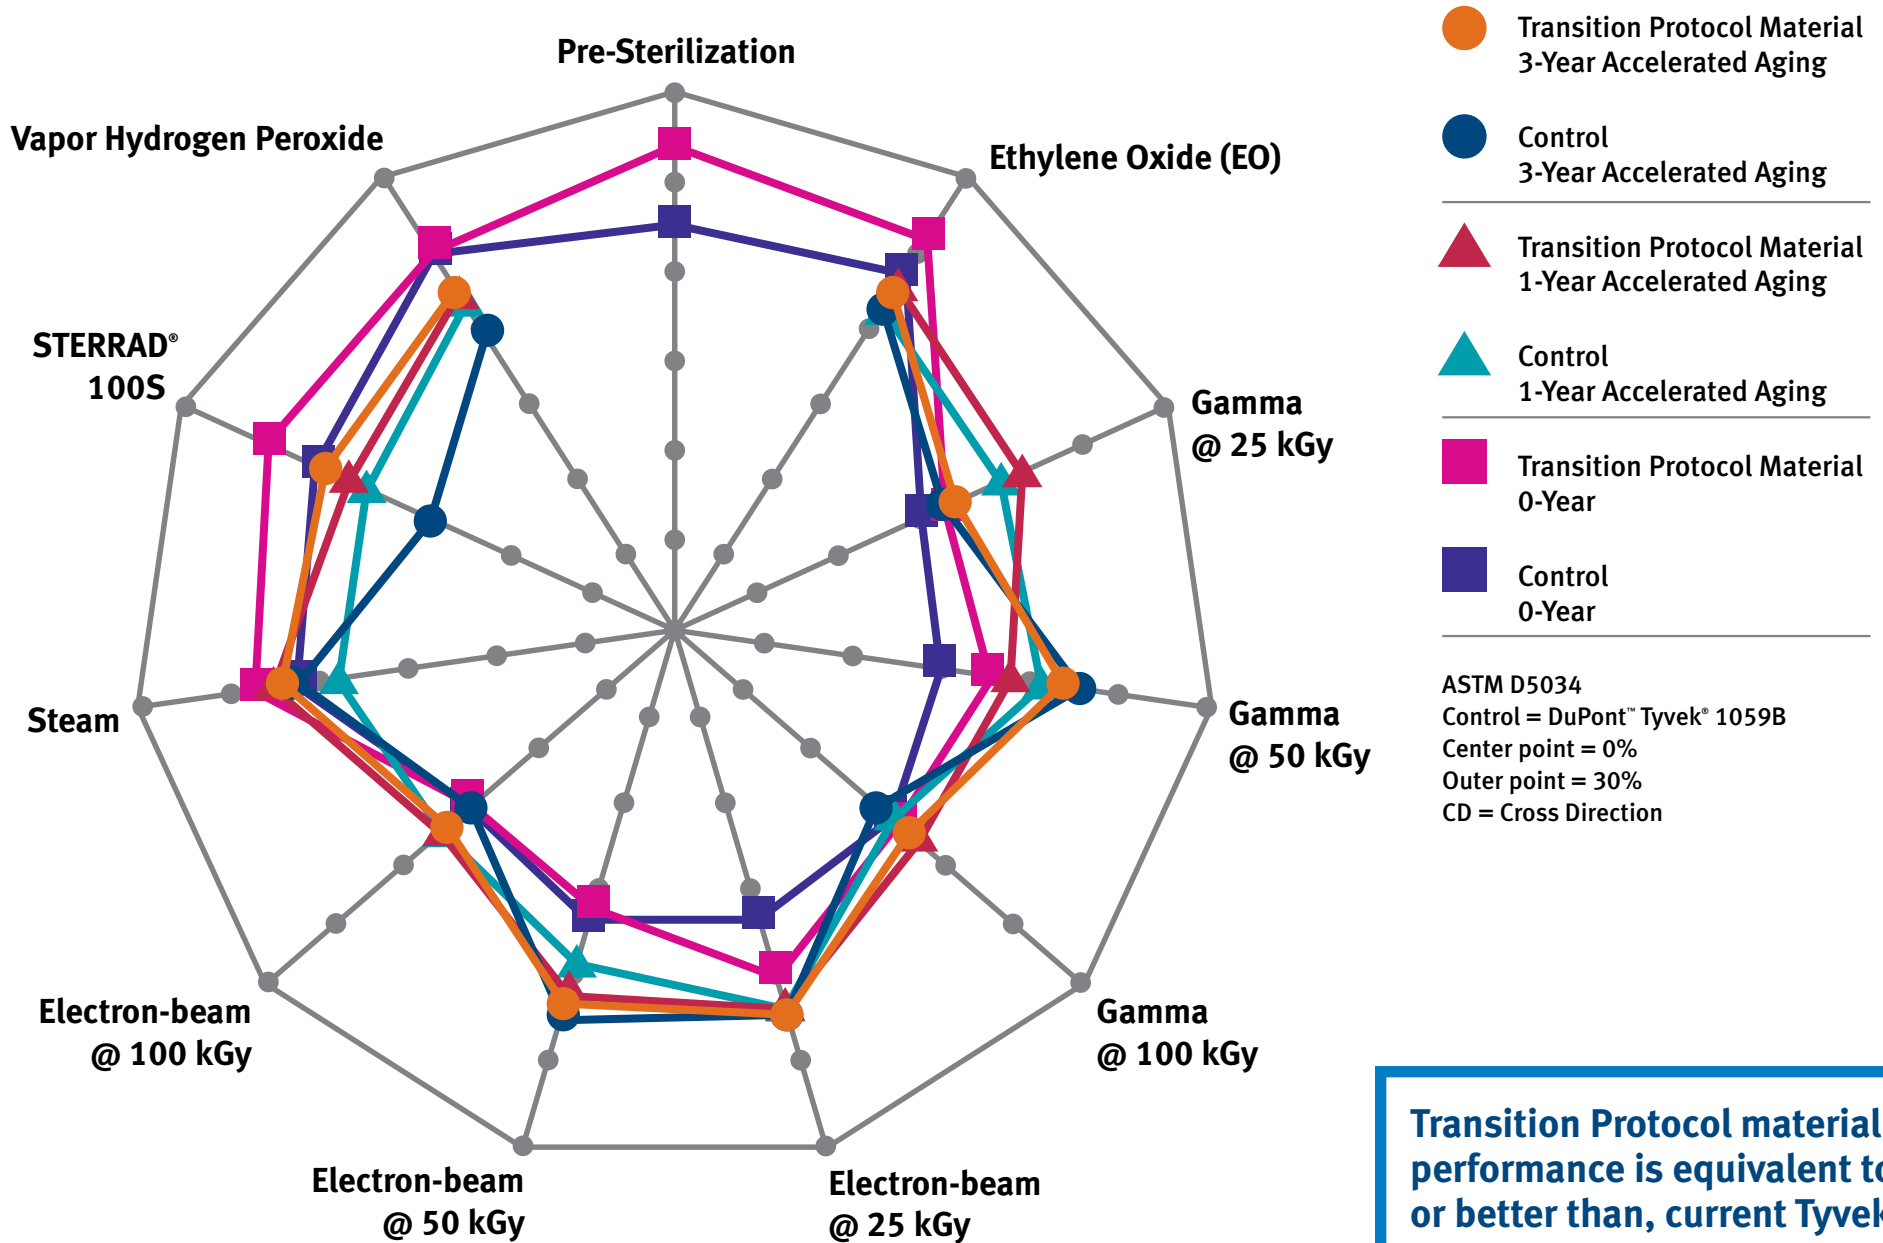

# Effects of Sterilization and 1- & 3-Year Accelerated Aging on Material Puncture Strength for 1059B



Tyvek.

