


High consistency rubber

Application and product selection guide



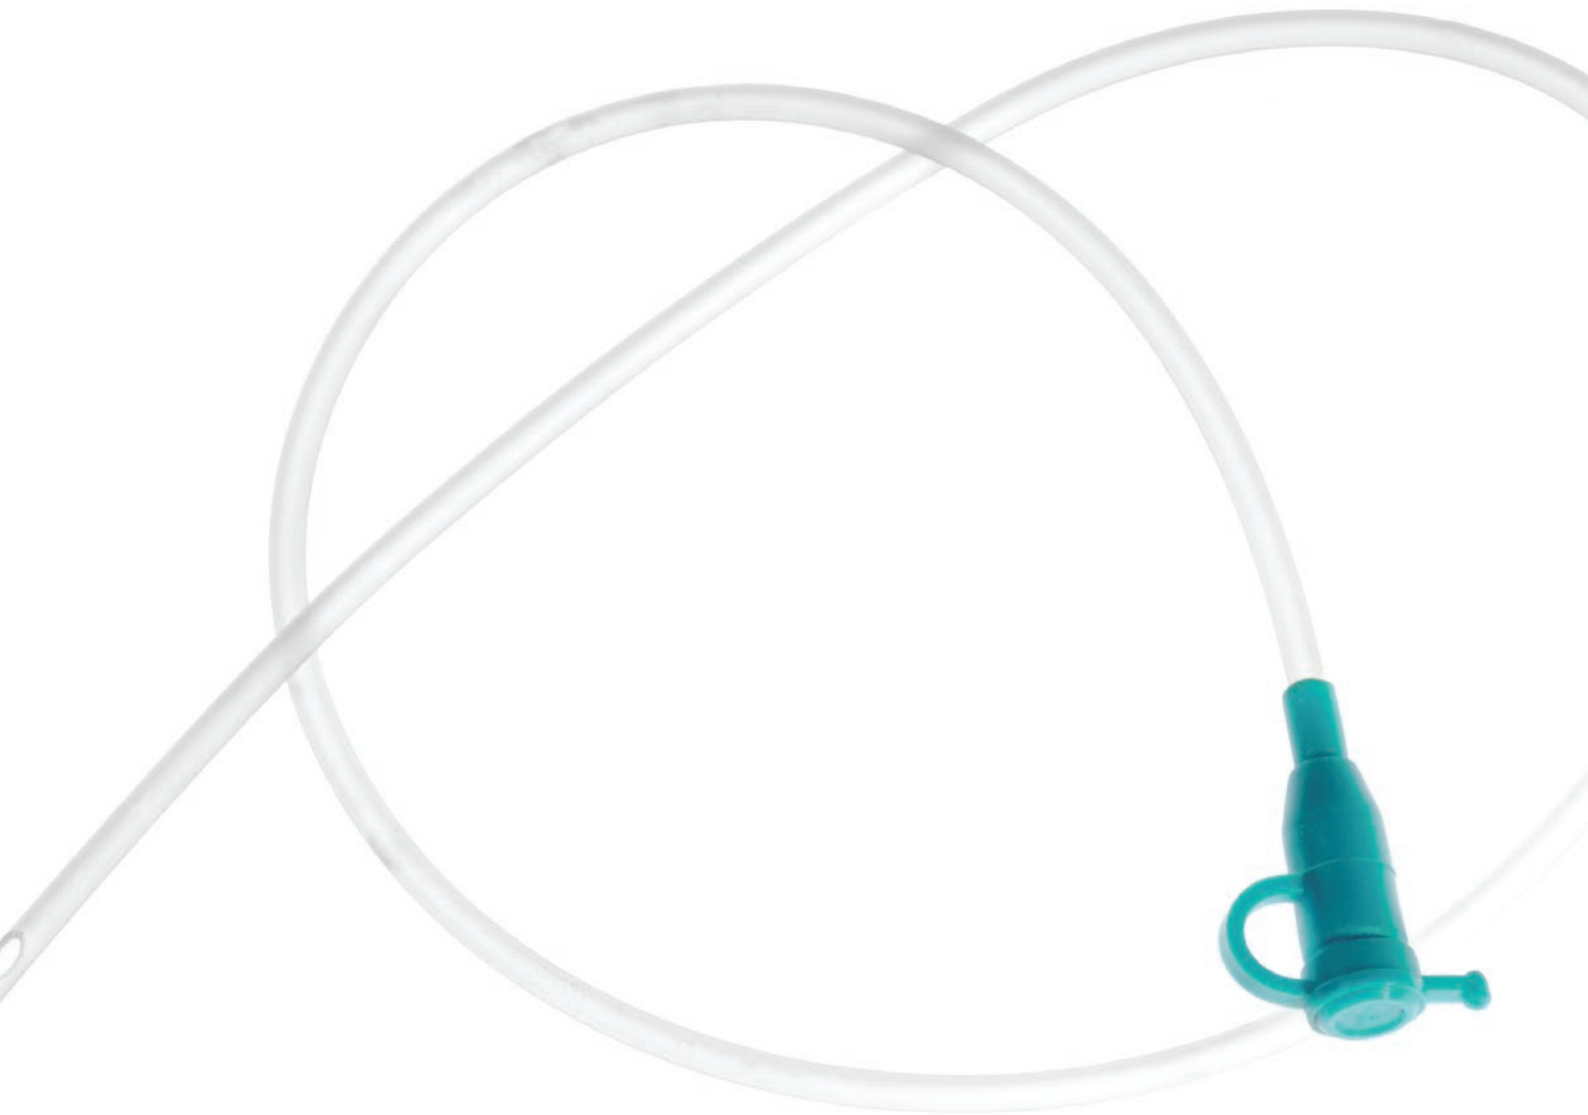

High consistency rubber (HCR)

HCRs are millable thermoset silicone elastomers that can be extruded continuously to form a desired size and shape before curing. Silicone tubing is an example.

Innovation meets expertise

You want to explore new directions and create the next generation of medical device technology. You have a powerful ally with DuPont™ Liveo™. When we are part of your team, you're backed by our expertise and our culture of discovery and innovation, which has been nurtured by six decades of proven performance. You'll find a depth of knowledge not just in silicone chemistry, but in the medical device industry, process technology, and regulatory compliance.

Benefits	Product Description	Typical Applications	Products	Biocompatibility Testing																					
				Cytotoxicity	Mutagenicity/Genotoxicity	Hemolysis	Skin Sensitization	Pyrogenicity (USP)	90-Day Implant	30-Day Implant	7-Day Implant	USP Class V and VI	Substance Soluble in Hexane	Volatile Matter	Food Grade Compliance*	Hardness, Shore A	Tensile Strength (MPa/psi)	Elongation at Break (%)	Tear Strength, Die B (kN/m/ppi)	Relative Density					
Liveo™ BioMedical Grade Elastomers • DMF (drug master file) access available upon request for select Liveo™ BioMedical Grade materials • Excellent batch-to-batch reproducibility for critical applications • Manufactured in a dedicated healthcare facility	Two-part (1:1 by weight), platinum-catalyzed, enhanced tear-resistance silicone elastomers	• Fabrication of extruded parts • Fabrication of molded medical/surgical/diagnostic devices and components	Liveo™ Q7-4720 BioMedical Grade ETR Elastomer ¹	•	•	•	•	•	•	•	•	•	•	•	•	•	•	23	8.9/1300	1310	31.6/180	1.11			
			Liveo™ Q7-4735 BioMedical Grade ETR Elastomer ¹	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	36	9.3/1350	1180	36.8/210	1.12	
			Liveo™ Q7-4750 BioMedical Grade ETR Elastomer ¹	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	50	10.0/1450	930	45.6/260	1.16
			Liveo™ Q7-4765 BioMedical Grade ETR Elastomer ¹	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	65	8.0/1160	900	45.6/260	1.20
			Liveo™ Q7-4780 BioMedical Grade ETR Elastomer ¹	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	77	7.8/1130	660	42.1/240	1.20
Liveo™ BioMedical Grade Bases • DMF (drug master file) access available upon request for select Liveo™ BioMedical Grade materials • Must add peroxide	Two-part (1:1 by weight), platinum-catalyzed, enhanced tear-resistance silicone elastomers	• Fabrication of extruded parts • Fabrication of molded medical/surgical/diagnostic devices and components	Liveo™ Q7-4535 BioMedical Grade ETR Elastomer ^{1,2}	•	•	•	•	•	•	•	•	•	•	•	•	•	•	36	8.1/1180	830	24.6/140	1.12			
			Liveo™ Q7-4550 BioMedical Grade ETR Elastomer ^{1,2}	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	48	9.3/1360	680	31.6/180	1.16	
Liveo™ C6 Series Elastomers • Highly reproducible and stable materials • Manufactured in a dedicated healthcare facility • Improved cost efficiency	Two-part (1:1 by weight), platinum-catalyzed, enhanced tear-resistance silicone elastomers	• Fabrication of extruded parts • Fabrication of molded medical/surgical/diagnostic devices and components	Liveo™ C6-135 Elastomer	•						•	•	•	•	•	•	•	•	36	8.2/1200	1120	35.1/200	1.12			
			Liveo™ C6-150 Elastomer	•								•	•	•	•	•	•	•	•	50	10.6/1540	980	42.1/240	1.16	
			Liveo™ C6-165 Elastomer	•									•	•	•	•	•	•	•	61	8.0/1170	940	42.1/240	1.21	
			Liveo™ C6-180 Elastomer	•										•	•	•	•	•	•	77	7.2/1050	610	38.6/220	1.21	
Liveo™ C6 Series Elastomers • Must add peroxide	One-part, high-consistency rubber base	• Fabrication of extruded parts • Fabrication of molded medical/surgical/diagnostic devices and components	Liveo™ C6-235 Elastomer ²	•														37	7.5/1100	810	21.1/120	1.12			
			Liveo™ C6-250 Elastomer ²	•																49	8.2/1200	530	26.3/150	1.16	
			Liveo™ C6-265 Elastomer ²	•																66	8.2/1200	560	35.1/200	1.20	
Liveo™ QP1 Elastomers • Base, must add curatives	One-part, high-consistency rubber base	• Fabrication of extruded parts • Fabrication of molded medical/surgical/diagnostic devices and components	Liveo™ QP1-30 Silicone Elastomer ³	•														28	9.5/1390	790	12.3/70	1.09			
			Liveo™ QP1-50 Silicone Elastomer ³	•																48	11.8/1720	545	15.8/90	1.13	
			Liveo™ QP1-60 Silicone Elastomer ³	•																57	13.0/1890	535	21.1/120	1.16	
			Liveo™ QP1-70 Silicone Elastomer ³	•																68	12.6/1835	470	24.6/140	1.20	
Liveo™ C6 Series Elastomers • Low hysteresis	Two-part (1:1 by weight), platinum-catalyzed, enhanced tear-resistance silicone elastomers	• Fabrication of extruded parts • Fabrication of molded medical/surgical/diagnostic devices and components	Liveo™ C6-350 LH Elastomer	•														49	8.5/1240	730	38.6/220	1.15			

¹ Use of this material for implantation ≥ 30 days requires indemnification
² 1.0 parts Di(2,4-Dichlorobenzoil) peroxide compounded with 100 parts base molded 5 min at 115°C (240°F)
³ 1.2 parts Di(2,4-Dichlorobenzoil) peroxide compounded with 100 parts base molded 5 min at 115°C (240°F)

* Contact your DuPont representative for area-specific information



To learn more about DuPont's healthcare solutions visit:
www.dupont.com/healthcare.html

For country-level information, visit:
www.dupont.com/corporate-functions/our-company/global-locations.html



CAUTION: DO NOT USE DUPONT MATERIALS IN MEDICAL APPLICATIONS INVOLVING PERMANENT IMPLANTATION IN THE HUMAN BODY OR PERMANENT CONTACT WITH INTERNAL BODILY FLUIDS OR TISSUES. DO NOT USE DUPONT MATERIALS IN MEDICAL APPLICATIONS INVOLVING BRIEF OR TEMPORARY IMPLANTATION IN THE HUMAN BODY OR PERMANENT CONTACT WITH INTERNAL BODILY FLUIDS OR TISSUES UNLESS THE MATERIAL HAS BEEN PROVIDED DIRECTLY BY DUPONT UNDER A CONTRACT THAT EXPRESSLY ACKNOWLEDGES THE CONTEMPLATED USE.

The information, suggestions and data contained herein are intended only as an informational guide to assist you in making preliminary selections of materials and are not intended to be all-inclusive or final. Because DuPont cannot anticipate or control the many different conditions under which this information, data, suggestions or materials may be used, DuPont does not guarantee the applicability or the accuracy of this information or the suitability of the information, data, suggestions, or materials in any given situation. The information, data, or suggestions are not intended to substitute for any testing you may need to conduct to determine for yourself the suitability of a particular material for a particular purpose. DuPont makes no guarantee of results and assumes no obligation or liability whatsoever in connection with this information. Such information, data or suggestions are to be used and relied upon at user's own discretion and risk. DuPont makes no warranties, express or implied, and disclaims any and all direct and indirect liability for damages or losses resulting from or relating to the use of any information, suggestion, data, or materials described herein. Statements concerning the use of the products or formulations described herein are not to be construed as recommending the infringement of any patent, copyright, designs or other intellectual property and no liability for infringement arising out of such use is assumed by DuPont. None of this information is to be considered as a license to operate under, or recommendation to infringe, any patents.

DuPont reserves the right not to sell Special Control and Premium Control products for selected applications.

Although these products are tested against certain USP Class VI and ISO 10993 standards, DuPont makes no representation or warranty of suitability of its products for particular healthcare or medical applications or any other representations or warranties based on such testing.

The information set forth herein is furnished free of charge and is based on technical data that DuPont believes to be reliable. It is intended for use by persons having technical skill at their own discretion and risk. DuPont makes no warranties, express or implied, and assumes no liability in connection with any use of this information.

DuPont™, the DuPont Oval Logo, and all products, unless otherwise noted, denoted with ™, SM or © are trademarks, service marks or registered trademarks of affiliates of DuPont de Nemours, Inc.

© 2020 DuPont de Nemours, Inc. All rights reserved.

Form Number: 001-20383-CDP0820